


TCVGH Temperature Log

Internal (°C)

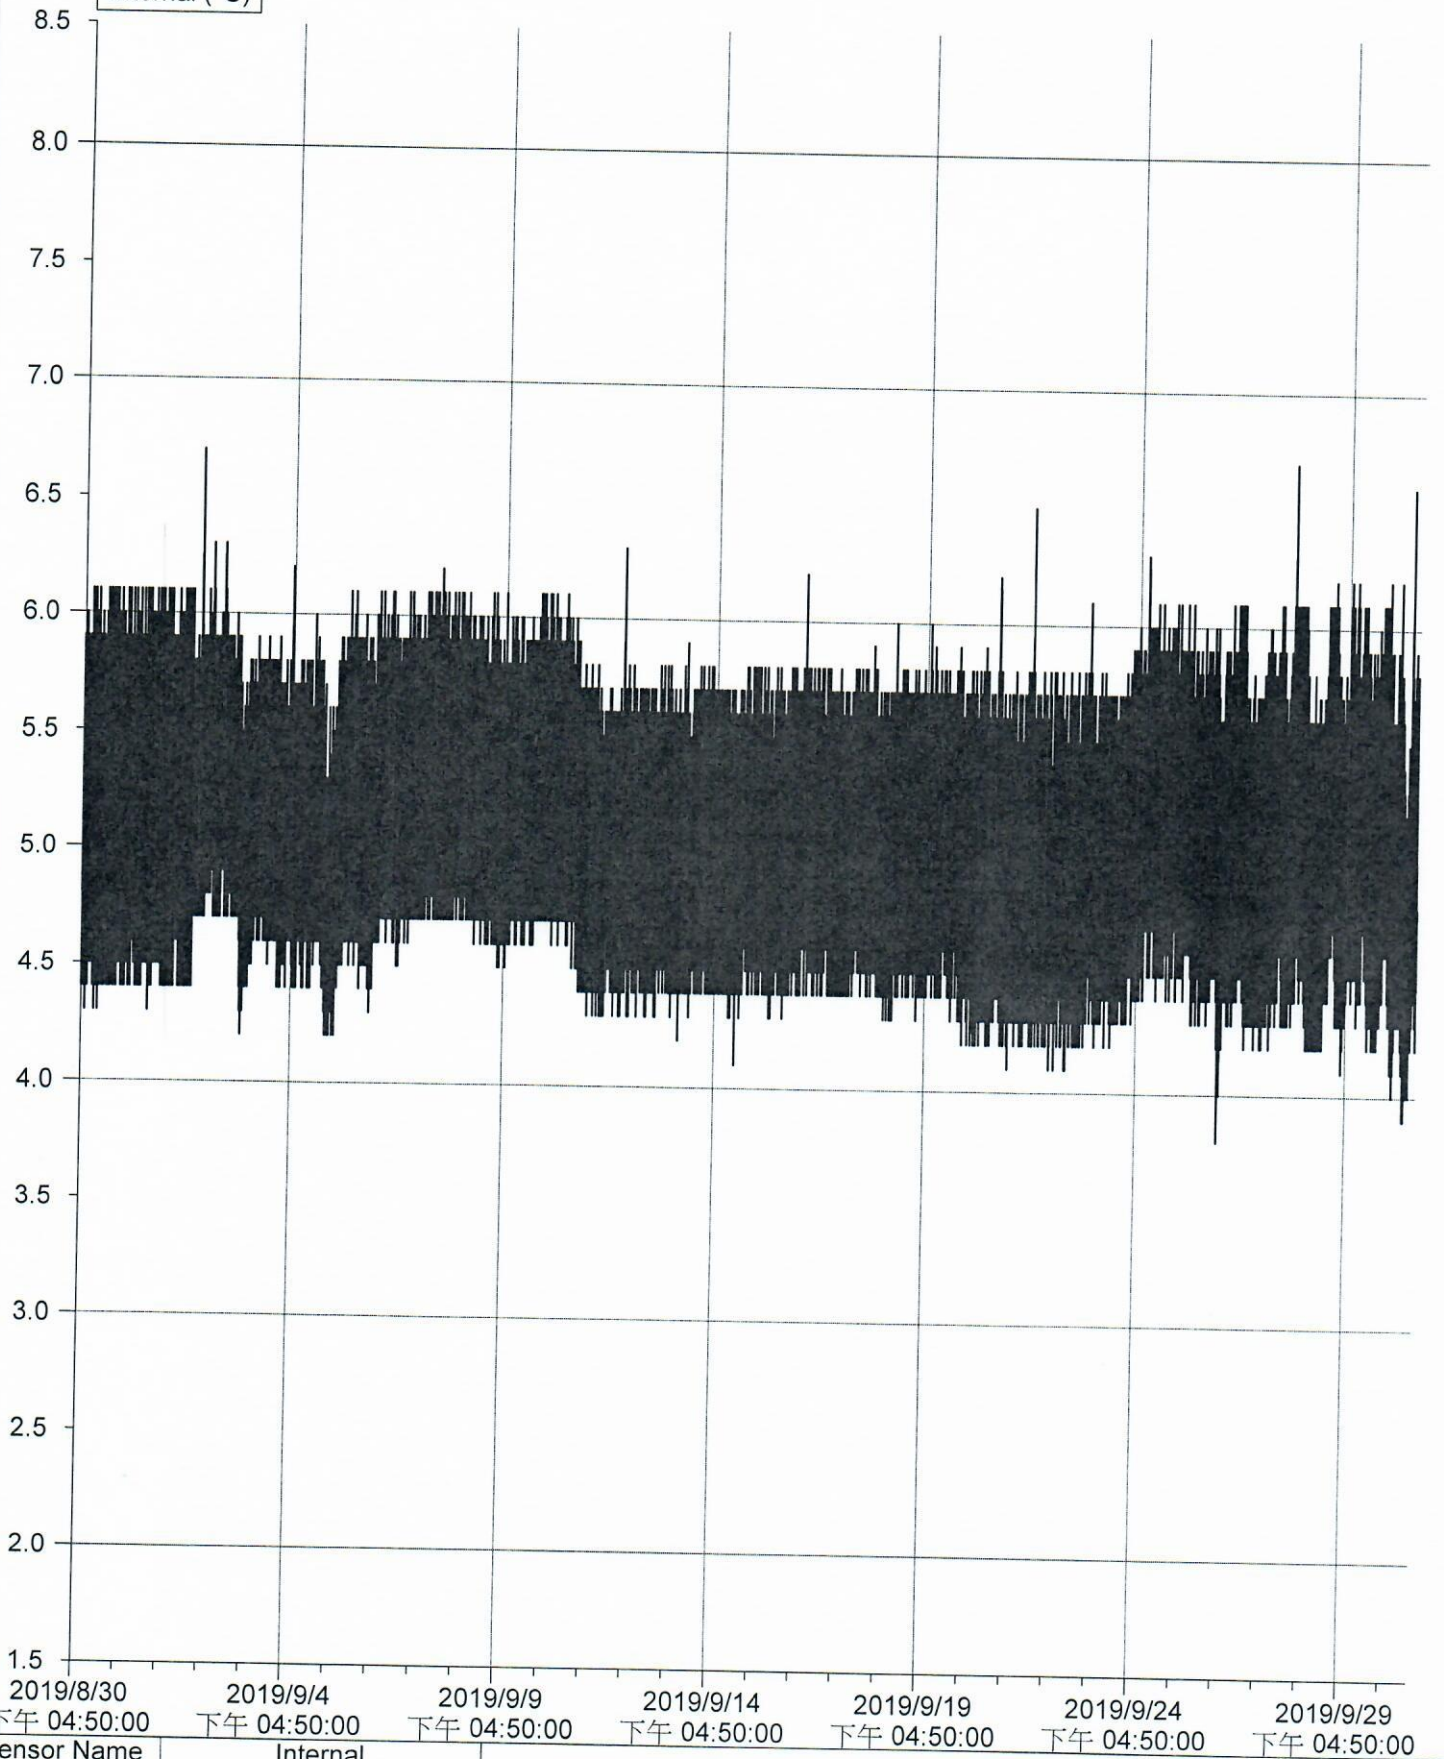

2019/8/30 下午 04:50:00 2019/9/4 下午 04:50:00 2019/9/9 下午 04:50:00 2019/9/14 下午 04:50:00 2019/9/19 下午 04:50:00 2019/9/24 下午 04:50:00 2019/9/29 下午 04:50:00

Sensor Name	Internal
Legend	
Description	PHCL-C001
Serial Number	1803-0047
Product Code	EI-IN-D-32-L
Start	2019/8/30 下午 04:50:00
Finish	2019/10/1 上午 09:00:00
Sensor Range	-40.5 to 70.4 °C
Specification	2.0 to 8.0 °C
Average	5.1 °C
Highest	6.7 °C
Lowest	3.8 °C

Nc-2mg

01 Oct 2019