


TCVGH Room Temperature Log

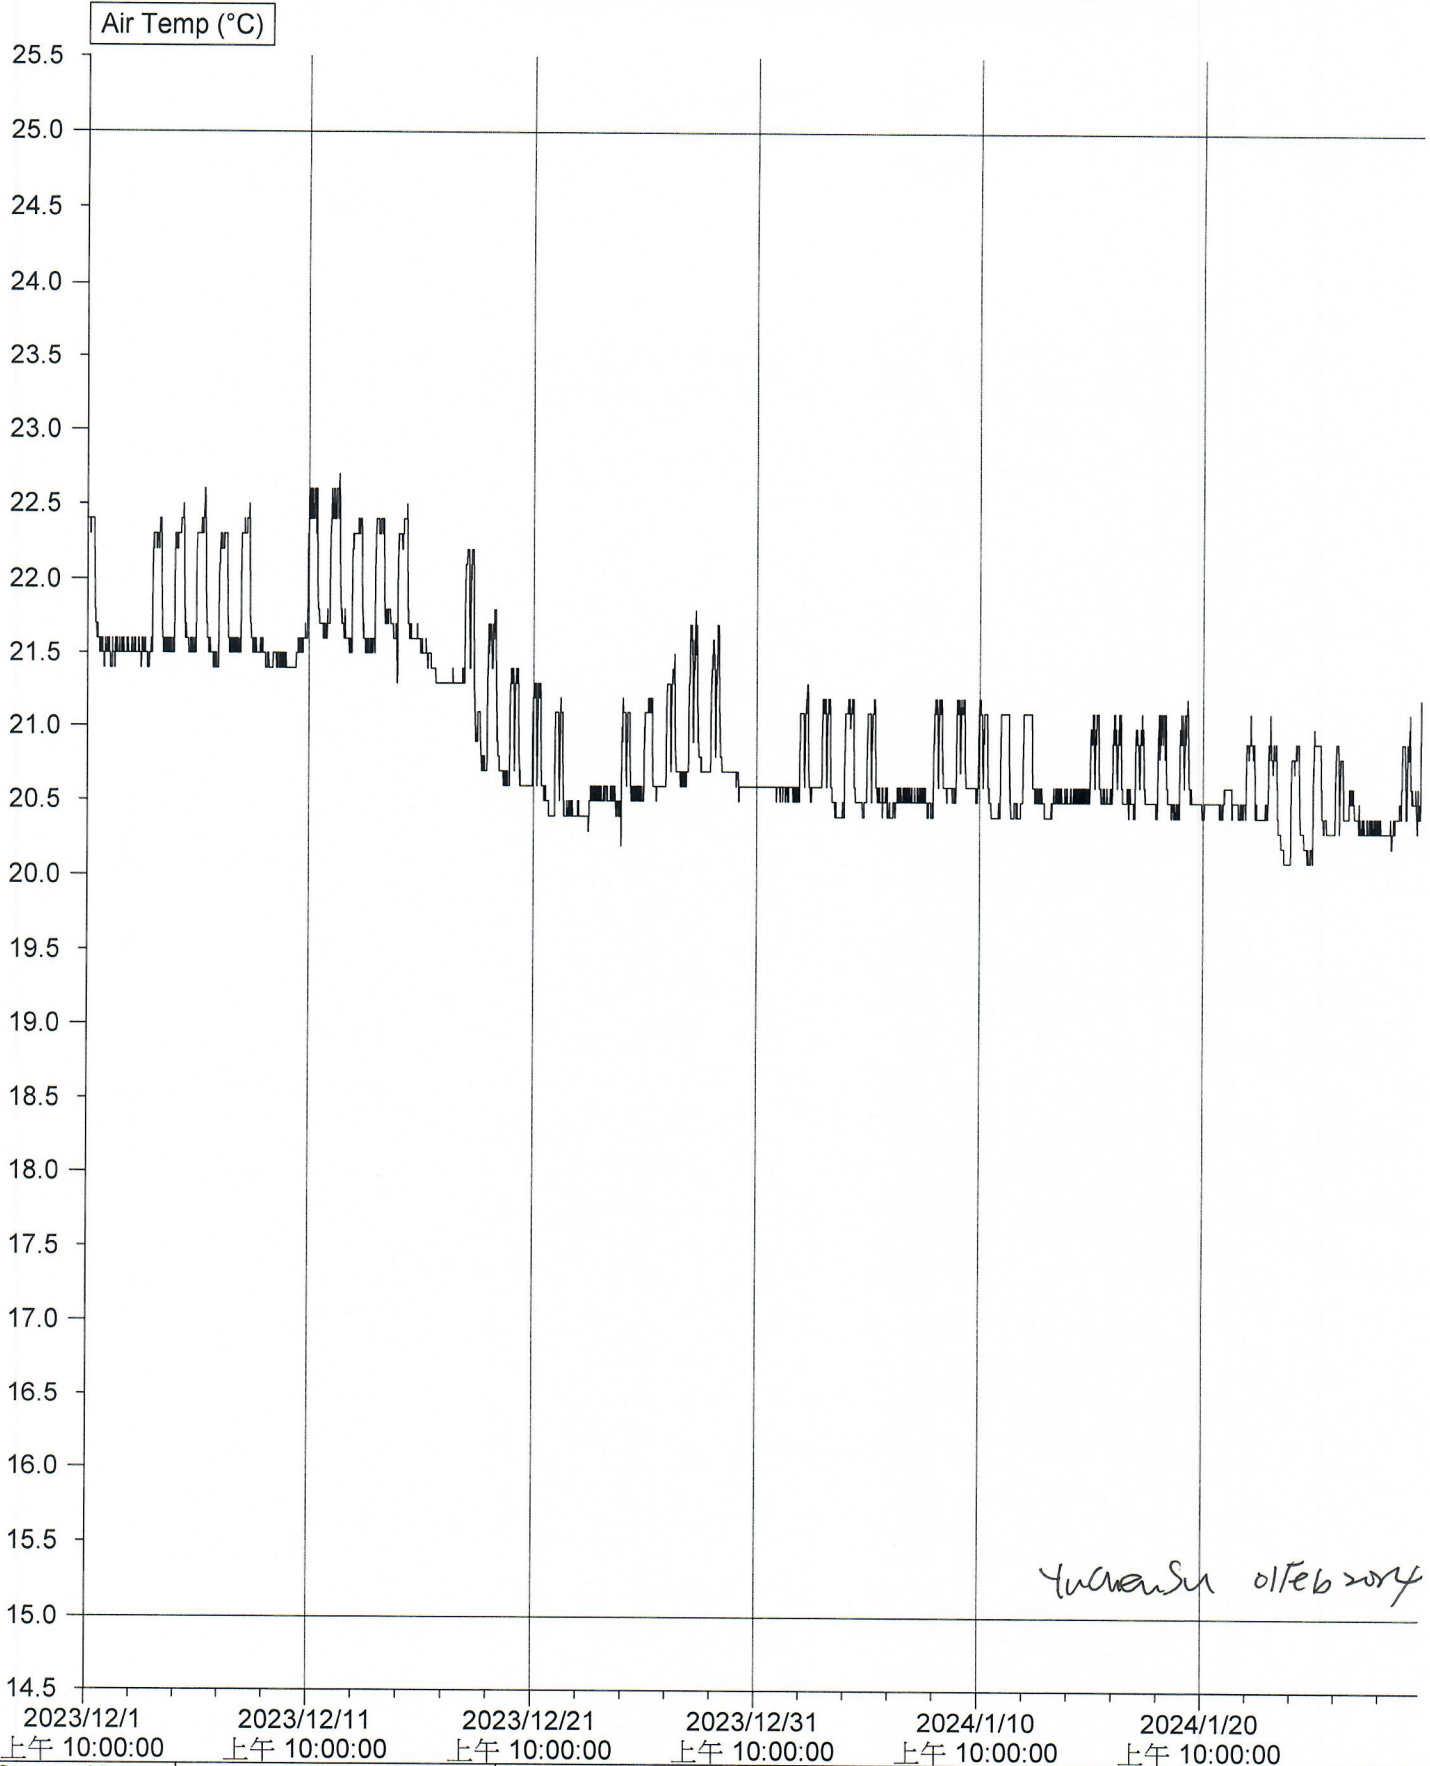


Yuchen Su 01Feb 2024

Sensor Name	Air Temp
Legend	
Description	Room temperature
Serial Number	1333-0016
Product Code	EI-HS-D-32-L
Start	2023/12/1 上午 10:00:00
Finish	2024/1/30 上午 05:40:00
Sensor Range	-40.5 to 70.4 °C
Specification	15.0 to 25.0 °C
Average	21.0 °C
Highest	22.7 °C
Lowest	20.1 °C

On January 30, 2024 at 08:10, the pharmacist discovered that the temperature recorder with serial number 1333-0016 had run out of battery. Consequently, back up temperature recorder with serial number 2106-0085 was provided for temperature recording after January 30. There is no temperature excursion events identified in the TCVGH cathical trial pharmacy room temperature.

TCVGH Room Temperature Log

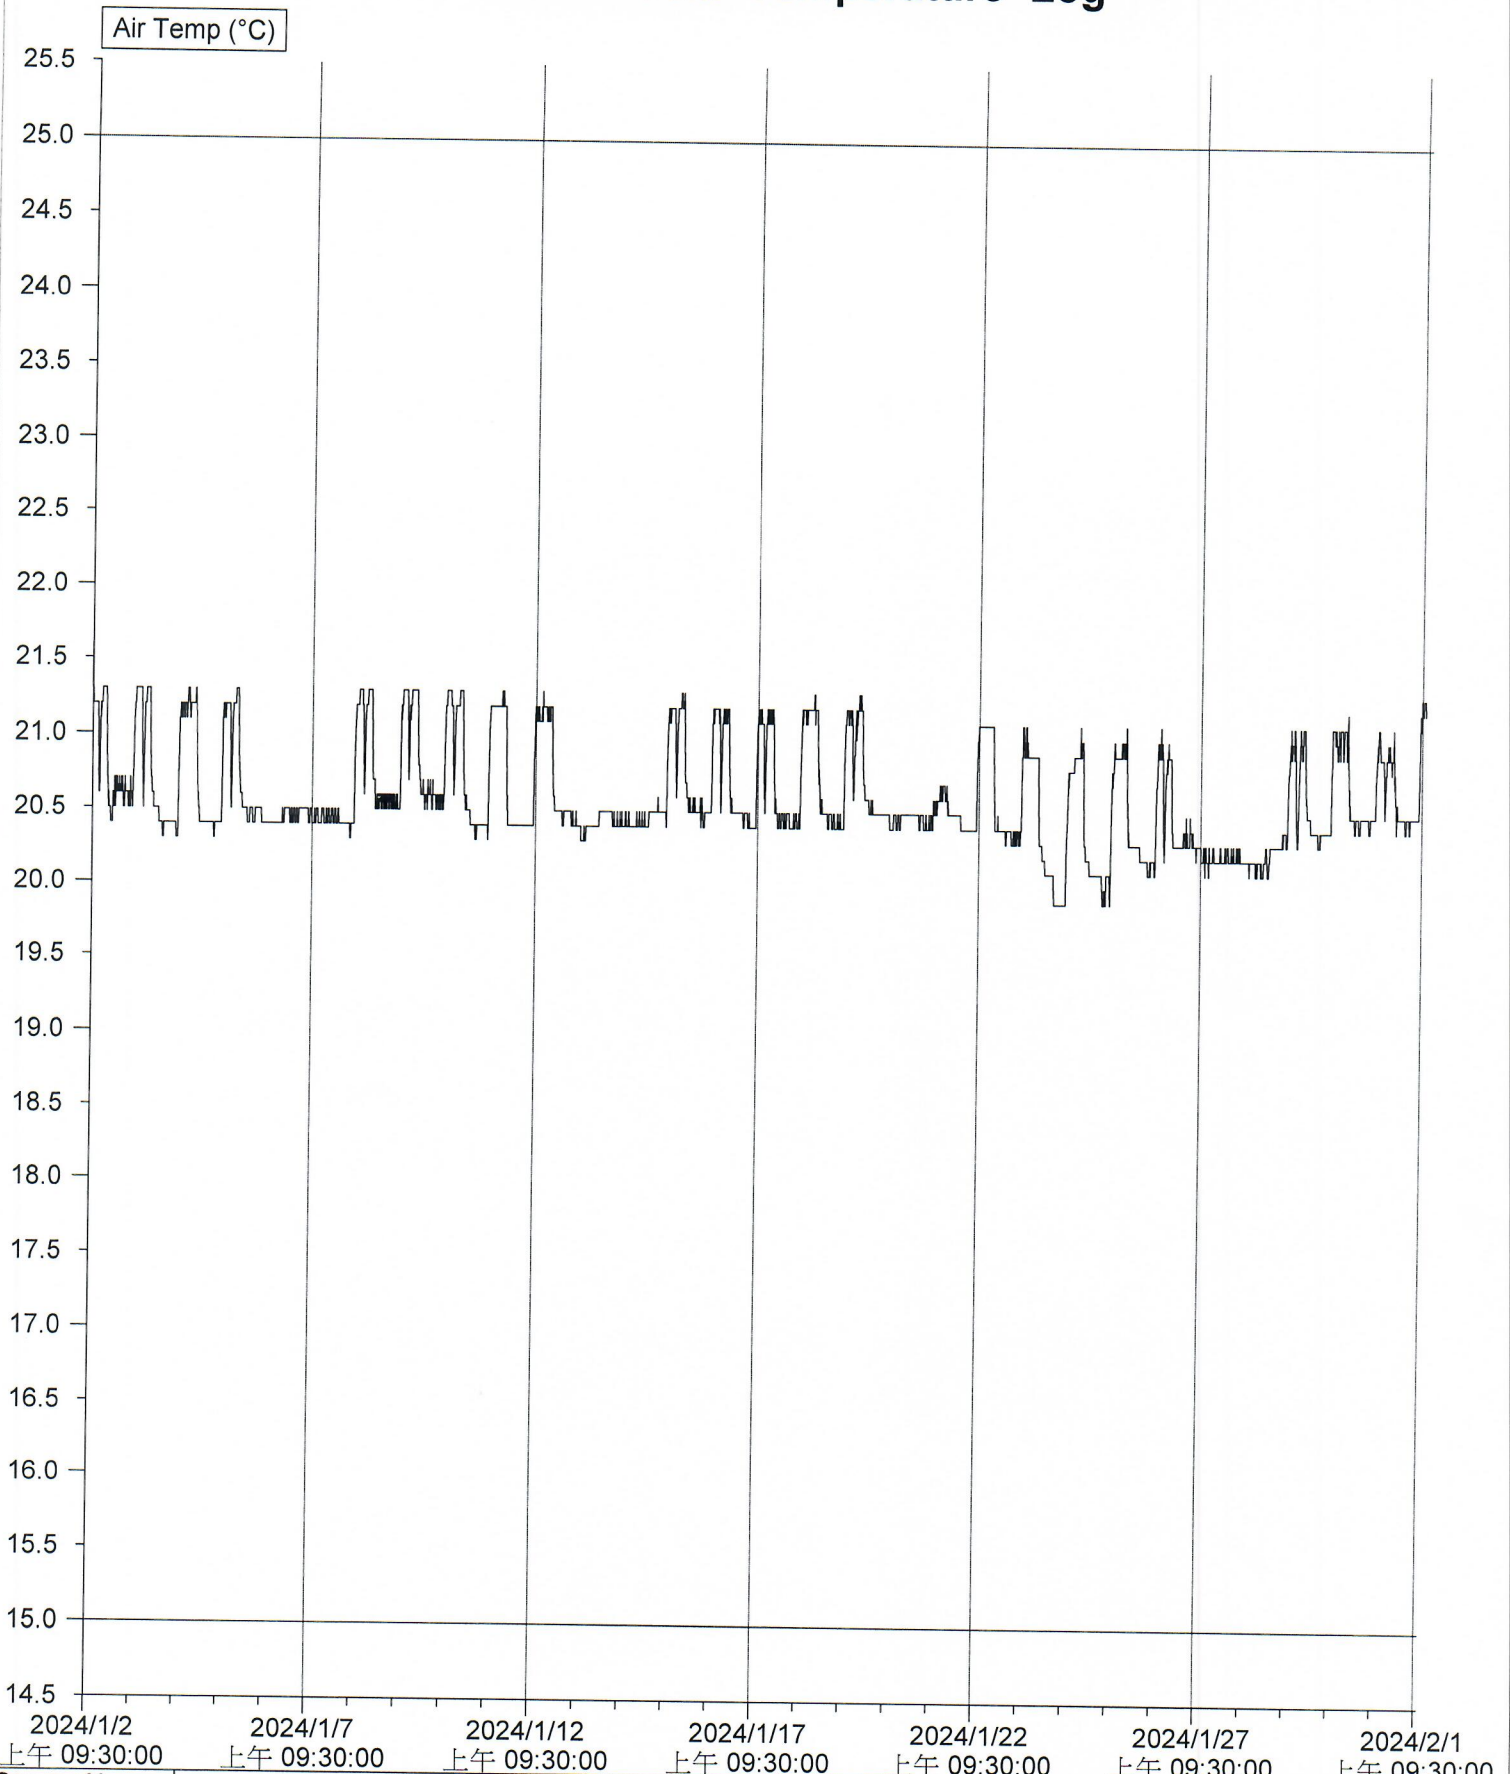

Sensor Name	Air Temp
Legend	
Description	Room Temperature 3
Serial Number	2106-0085
Product Code	EI-HS-D-32-L
Start	2024/1/2 上午 09:30:00
Finish	2024/2/1 上午 11:10:00
Sensor Range	-40.5 to 70.4 °C
Specification	15.0 to 25.0 °C
Average	20.6 °C
Highest	21.6 °C
Lowest	19.9 °C

Yuchen Su
01 Feb 2024